


Program: 9012
Name: CHLORINE
Calibration: $C = a + bA$
a: -0.071 b: 4.0671
Curve Fit $r^2 =$ 0.9987

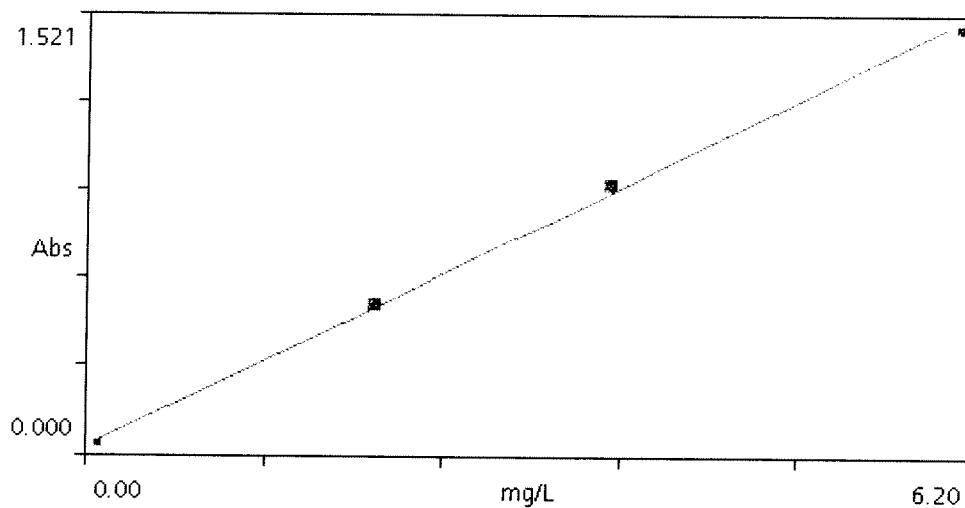

mg/L	Abs
0.0000	0.000
2.0000	0.520
3.7000	0.956
6.2000	1.521